



Centre 145

EINGEGANGEN
03. Feb. 2013
TQM

PT Distribution 346


Samples dispatched on: 8th January 2013

Results deadline: 1st February 2013

Bias plot: Distribution 343 - 346

Method: AC/MIA – on Dimension platform

Group Code: AC/MIA

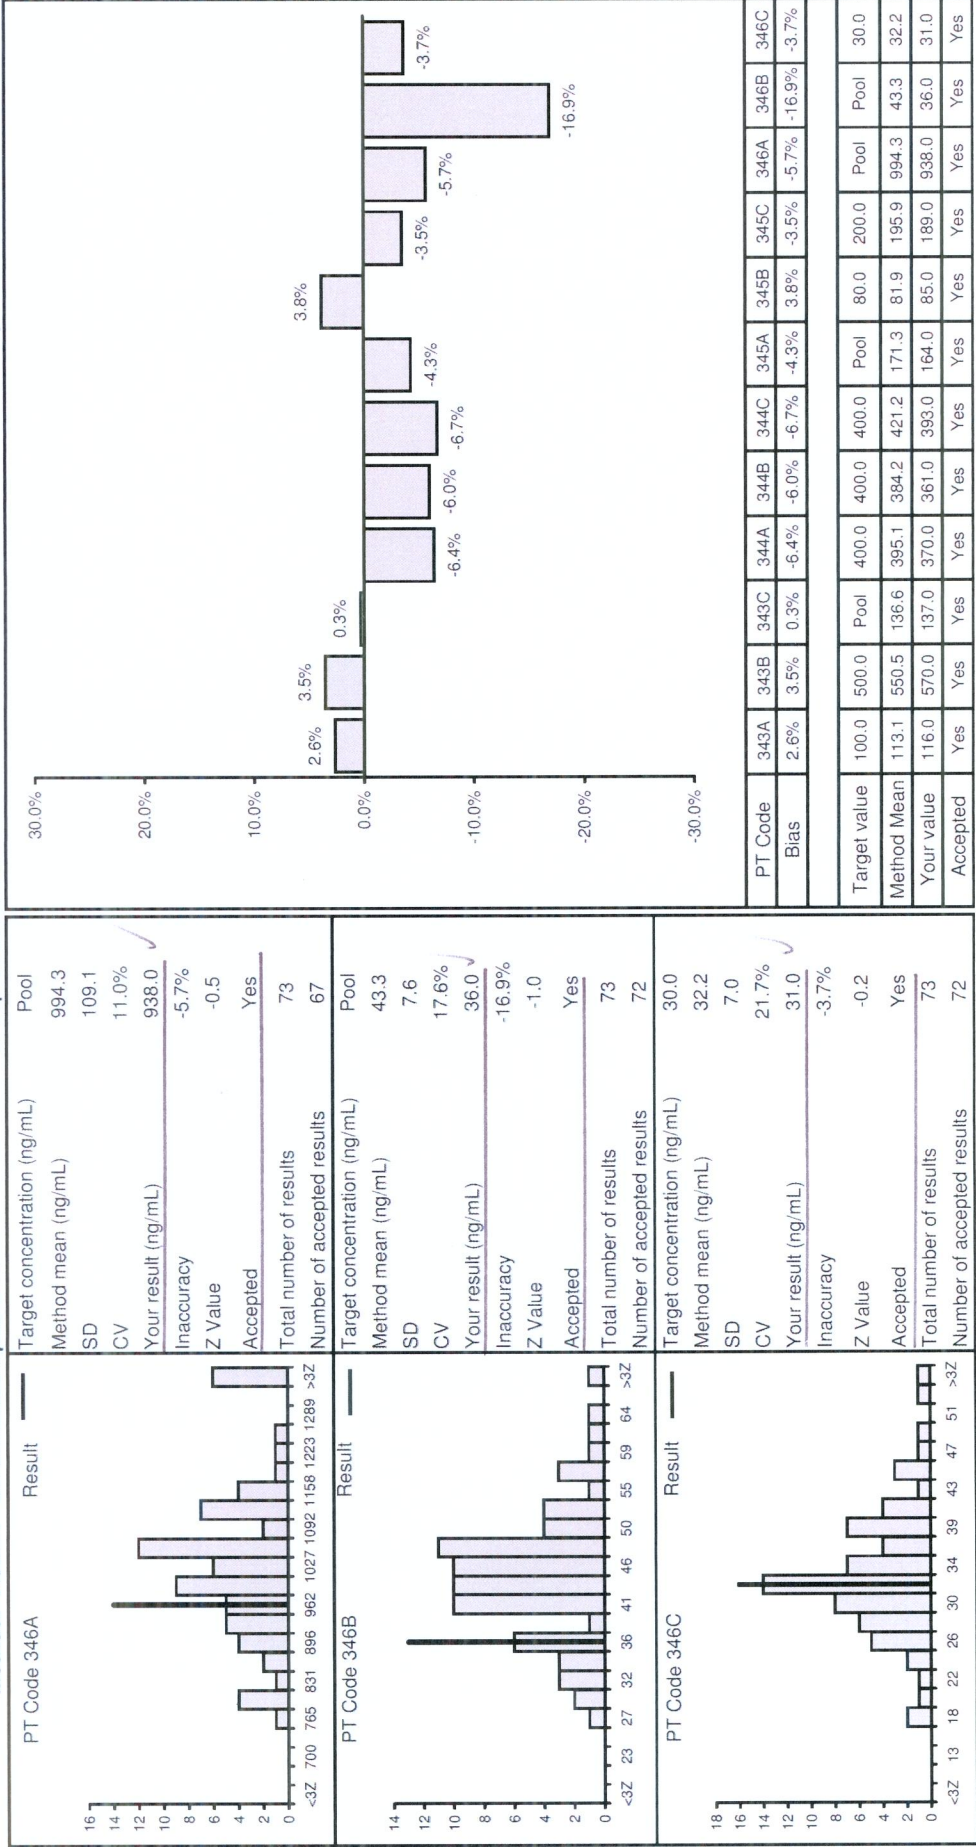

Target concentration (ng/mL)	Pool
Method mean (ng/mL)	994.3
SD	109.1
CV	11.0%
Your result (ng/mL)	938.0
Inaccuracy	-5.7%
Z Value	-0.5
Accepted	Yes
Total number of results	73
Number of accepted results	67

Target concentration (ng/mL)	Pool
Method mean (ng/mL)	43.3
SD	7.6
CV	17.6%
Your result (ng/mL)	36.0
Inaccuracy	-16.9%
Z Value	-1.0
Accepted	Yes
Total number of results	73
Number of accepted results	72

Target concentration (ng/mL)	Pool
Method mean (ng/mL)	30.0
SD	32.2
CV	7.0
Your result (ng/mL)	31.0
Inaccuracy	-3.7%
Z Value	-0.2
Accepted	Yes
Total number of results	73
Number of accepted results	72

