

EINGEGANGEN
 03. Juli 2013
 TQM

[Handwritten signature]

International proficiency testing scheme - Tacrolimus

Centre 1022



PT Distribution 217


Samples dispatched on: 4th June 2013

Results deadline: 28th June 2013


Method: CMIA - on Architect platform

Group Code: Architect


Bias plot: Distribution 214 - 217

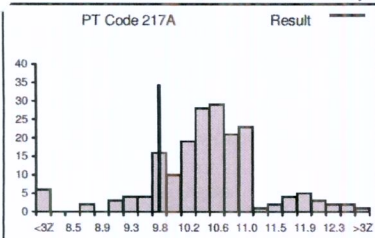


Target concentration (ng/mL)	10.0
Method mean (ng/mL)	10.4
SD	0.7
CV	6.7%
Your result (ng/mL)	9.7 ✓
Inaccuracy	-6.7%
Z Value	-1.0
Accepted	Yes
Total number of results	186
Number of accepted results	177

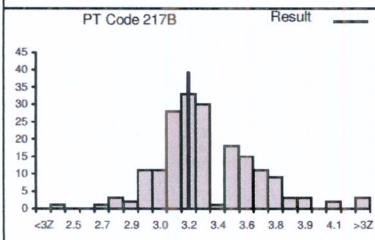

Target concentration (ng/mL)	3.0
Method mean (ng/mL)	3.3
SD	0.3
CV	9.1%
Your result (ng/mL)	3.2 ✓
Inaccuracy	-3.0%
Z Value	-0.3
Accepted	Yes
Total number of results	186
Number of accepted results	181

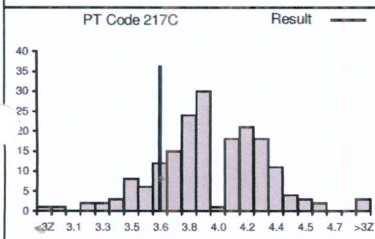

Target concentration (ng/mL)	4.0
Method mean (ng/mL)	3.9
SD	0.3
CV	7.7%
Your result (ng/mL)	3.6 ✓
Inaccuracy	-7.7%
Z Value	-1.0
Accepted	Yes
Total number of results	186
Number of accepted results	181

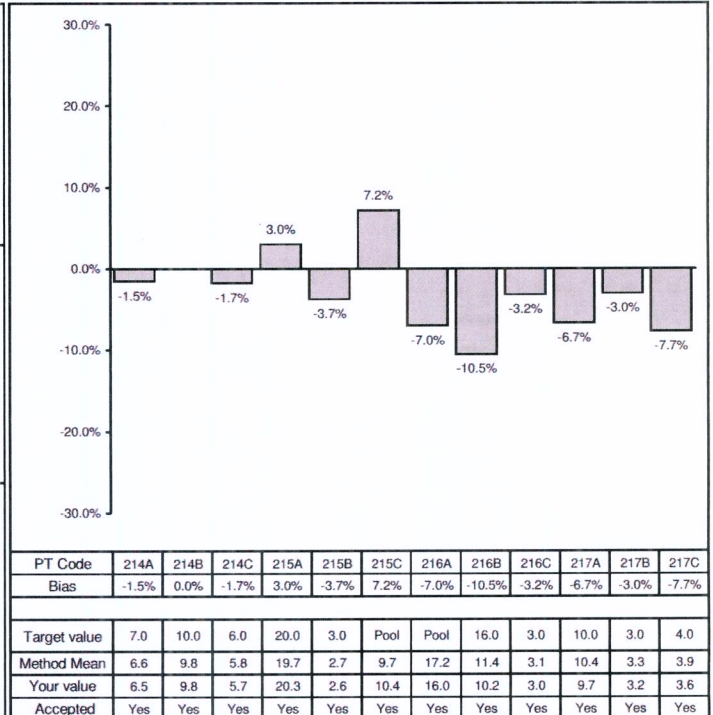

[Handwritten signature]