



EINGEGANGEN  
18 Juni  
TQM

Centre 4021


PT Distribution 84

Samples dispatched on: 05 May 2015  
Results deadline: 12 June 2015

Method: HPLC-MS or HPLC-MS/MS

Bias plot: Distribution 81 - 84

Group Code: HPLC

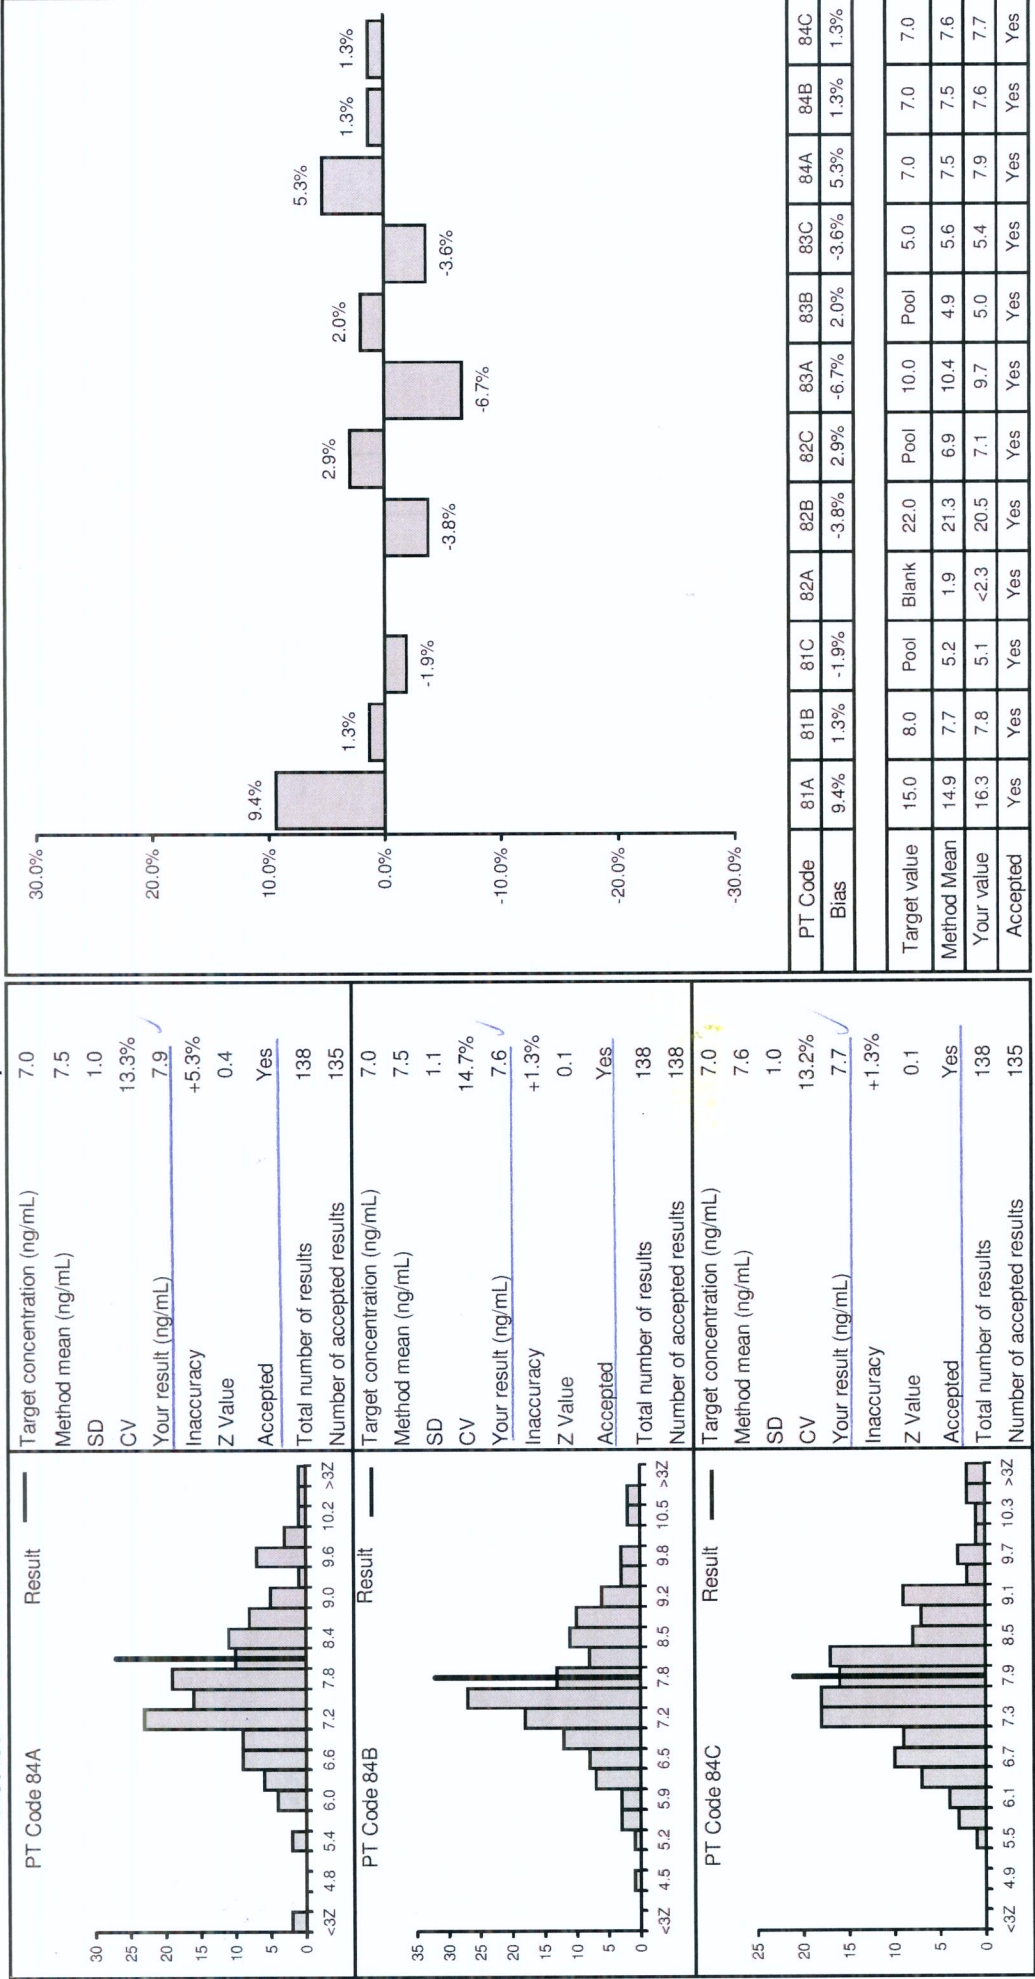

9/1